


CABINET

GERMAIN & MAUREAU

FONDÉ EN 1849

CONSEILS EN PROPRIÉTÉ INDUSTRIELLE



TELEX 370391 F
TÉL. (7) 860.24.93

LE BRITANNIA - TOUR C
20, BOULEVARD E.-DERUELLE
69003 LYON

BREVET D'INVENTION

PAYS : ETATS-UNIS

NUMÉRO : 4.663.720

DATE : 5 Mai 1987

TITRE : Procédé de réalisation d'une prothèse

TITULAIRE : DURET François
TERMOZ Christian

INVENTEUR :

PRIORITÉ :

DURÉE : 17 ANS

Continuation -in part

The

The Commissioner of Patents
and Trademarks

CABINET
GERMAIN & MAUREAU
CONSEILS EN PROPRIÉTÉ INDUSTRIELLE

BREVETS D'INVENTION, MARQUES ET MODÈLES

« LE BRITANNIA »

BOULEVARD EUGÈNE-DERUELLE - 69003 LYON
78 60 24 93 TÉLEX GERMAU 370391 F

HENNSON INTERNATIONAL
Chateau de Malissol
38200 VIENNE

Le 21 Mai 1987

avons l'honneur de vous remettre, inclus, les documents ci-dessous mentionnés.

DÉSIGNATION DES DOCUMENTS	OBJET	PAYS	NUMÉRO	DATE
PRE OFFICIEL	BREVET	ETATS-UNIS	4.663.720	5.5.1987



Commissioner of Patents and Trademarks

Melvinia Gary
Attest

The
United
States
of
America



The Commissioner of Patents and Trademarks

*Has received an application for a patent
for a new and useful invention. The title
and description of the invention are en-
closed. The requirements of law have
been complied with, and it has been de-
termined that a patent on the invention
shall be granted under the law.*

Therefore, this

United States Patent

*Grants to the person or persons having
title to this patent the right to exclude
others from making, using or selling the
invention throughout the United States
of America for the term of seventeen
years from the date of this patent, sub-
ject to the payment of maintenance fees
as provided by law.*

Ronald D. Zigg

Commissioner of Patents and Trademarks

Melvinia Gary
Attest

United States

Duret et al.

[54] **METHOD OF
MAKING A
DENTAL PRO**

[76] **Inventors: F
I
J
C**

[21] **Appl. No.: 6**

[22] **Filed: N**

Related

[63] **Continuation-
which is a co
1981, abandon**

[51] **Int. Cl.⁴**

[52] **U.S. Cl.**

[58] **Field of Search
356/347, :**

[56]

U.S. PA

3,749,493 7/197
3,943,278 3/197
4,324,546 4/198
4,385,360 5/198
4,411,626 10/198
4,464,052 8/198
4,575,805 3/198

FOREIGN

0040165 11/198
0091876 10/198

NOTICE

If the application for this patent was filed on or after December 12, 1980, maintenance fees are due three years and six months, seven years and six months, and eleven years and six months after the date of this grant, or within a grace period of six months thereafter upon payment of a surcharge as provided by law. The amount, number, and timing of the maintenance fees required may be changed by law or regulation.

[54] METHOD OF AND APPARATUS FOR MAKING A PROSTHESIS, ESPECIALLY A DENTAL PROSTHESIS

[76] Inventors: Francois Duret, Rue Paul Claude, Le Grand Lemps (Isere); Christian Termoz, 2, Place Victor Hugo, Grenoble (Isere), both of France

[21] Appl. No.: 673,655

[22] Filed: Nov. 21, 1984

Related U.S. Application Data

[63] Continuation-in-part of Ser. No. 560,776, Feb. 21, 1984, which is a continuation of Ser. No. 262,905, May 12, 1981, abandoned.

[51] Int. Cl.⁴ G06F 15/00; A61C 9/00

[52] U.S. Cl. 364/474; 433/214

[58] Field of Search 364/474, 168, 475; 356/347, 357, 358; 433/204, 213, 214, 223, 55, 68, 73

References Cited

U.S. PATENT DOCUMENTS

3,749,493	7/1973	Malovski	356/357
3,943,278	3/1976	Ramsey	356/357
4,324,546	4/1982	Heitlinger	433/213
4,385,360	5/1983	Yamada	364/475
4,411,626	10/1983	Becker	364/168
4,464,052	8/1984	Neumann	356/347
4,575,805	3/1986	Moermann	364/475

FOREIGN PATENT DOCUMENTS

0040165	11/1981	European Pat. Off.	433/214
0091876	10/1983	European Pat. Off.	433/214

OTHER PUBLICATIONS

EP0040165; Translation into English; 11-18-81.

EP0091876; English Translation; 10-19-83.

Primary Examiner—Jerry Smith

Assistant Examiner—Allen MacDonald

Attorney, Agent, or Firm—Karl F. Ross; Herbert Dubno

[57] ABSTRACT

A method of making a dental prosthesis in which data representing standard tooth shapes and sizes, relationships between teeth and adjacent and occlusive teeth and characteristics for securing a prosthesis to a prepared site, and machining instructions for shaping a blank to the configuration of a dental prosthesis for direct implantation are stored in a computer memory. After preparing a site in the mouth of a patient to receive a dental prosthesis, the dental surgeon projects optically a grating upon said site in the mouth of the patient and generates an interference pattern representing a holistic impression of said site and its relationship to adjacent structures. The interference pattern is converted into data along x,y,z coordinates in a cartesian coordinate system representing machining of a blank to fit said site and matching data obtained by comparing the impression with the computer standards are used to select a best-fit shape and size. A machine tool is numerically controlled with the x,y,z coordinate data and x,y,z coordinate data from the match made by the computer and representing the shape and size of the prosthesis to totally and three-dimensionally fabricate said prosthesis in said machine tool.

7 Claims, 21 Drawing Figures

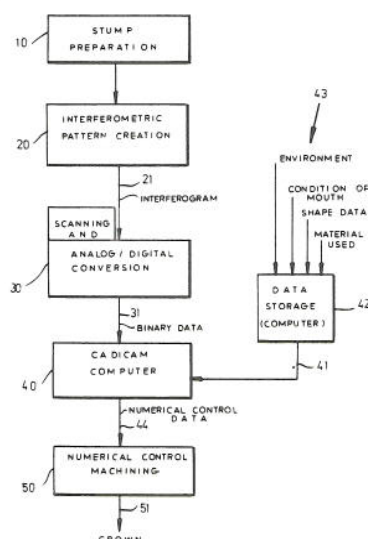


FIG.1

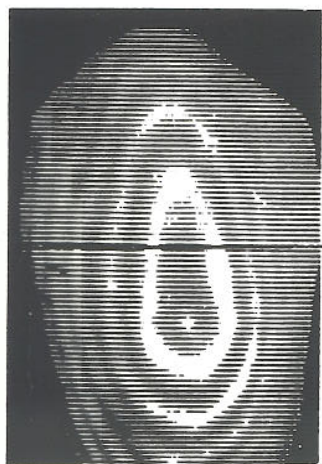


FIG.2



FIG.3

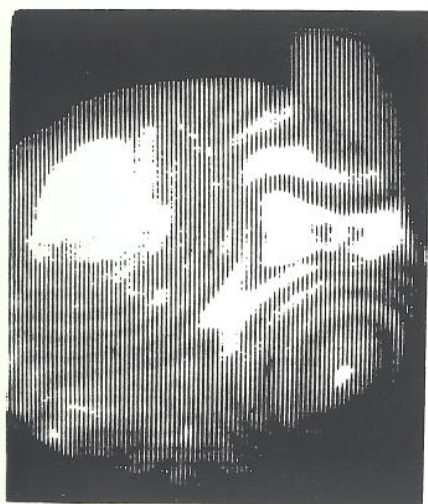


FIG.4



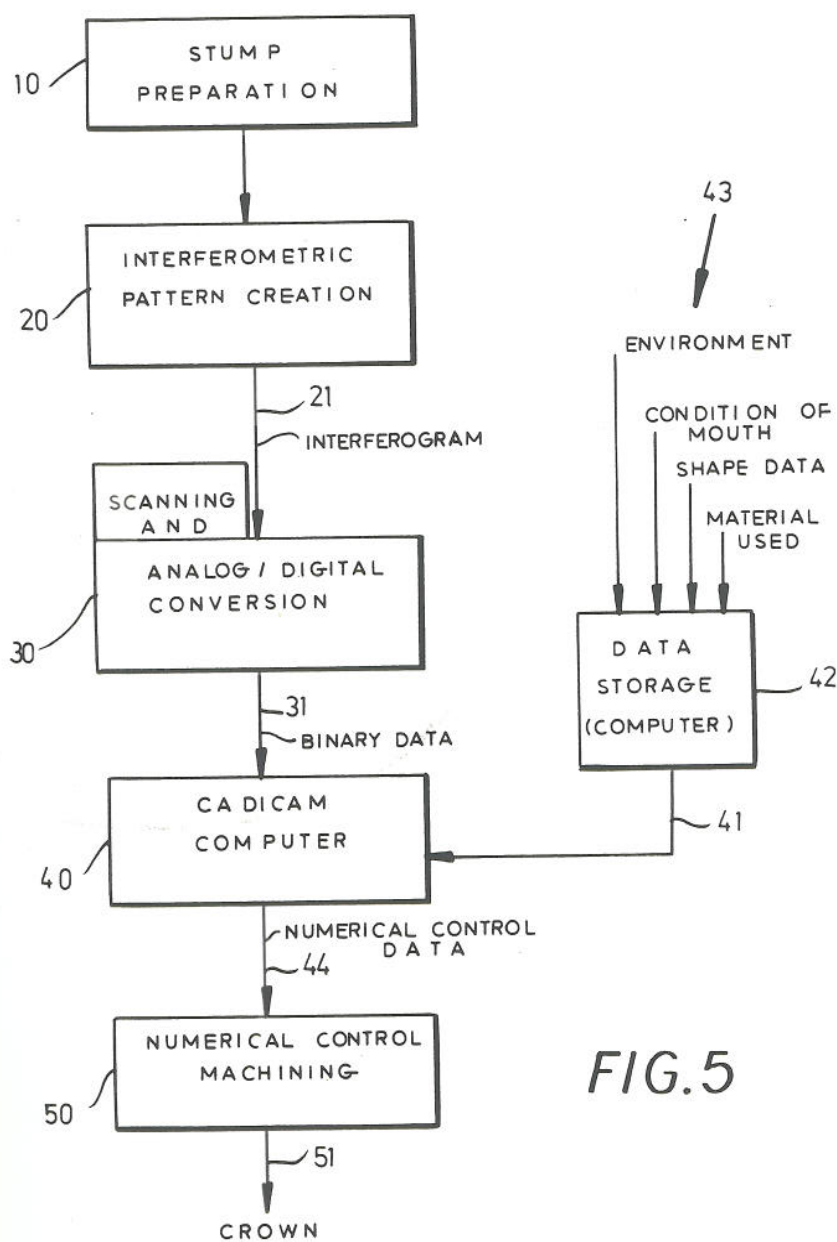
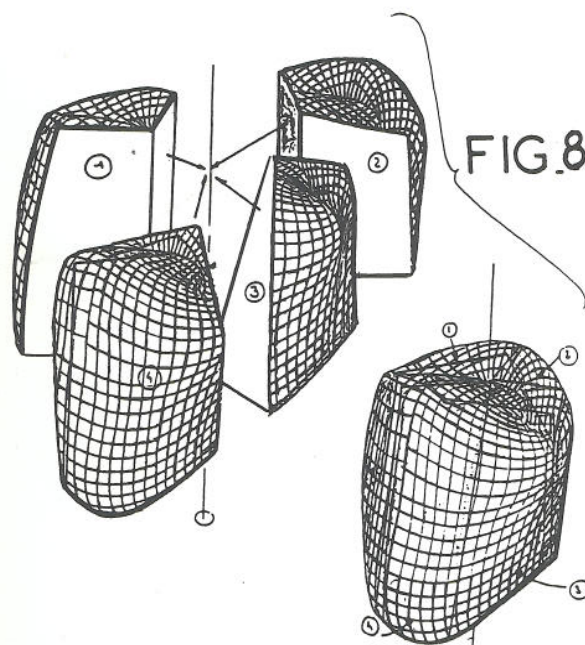
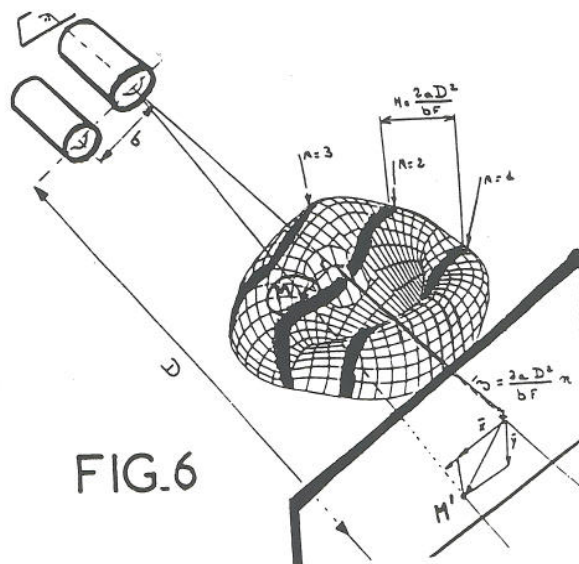


FIG. 5



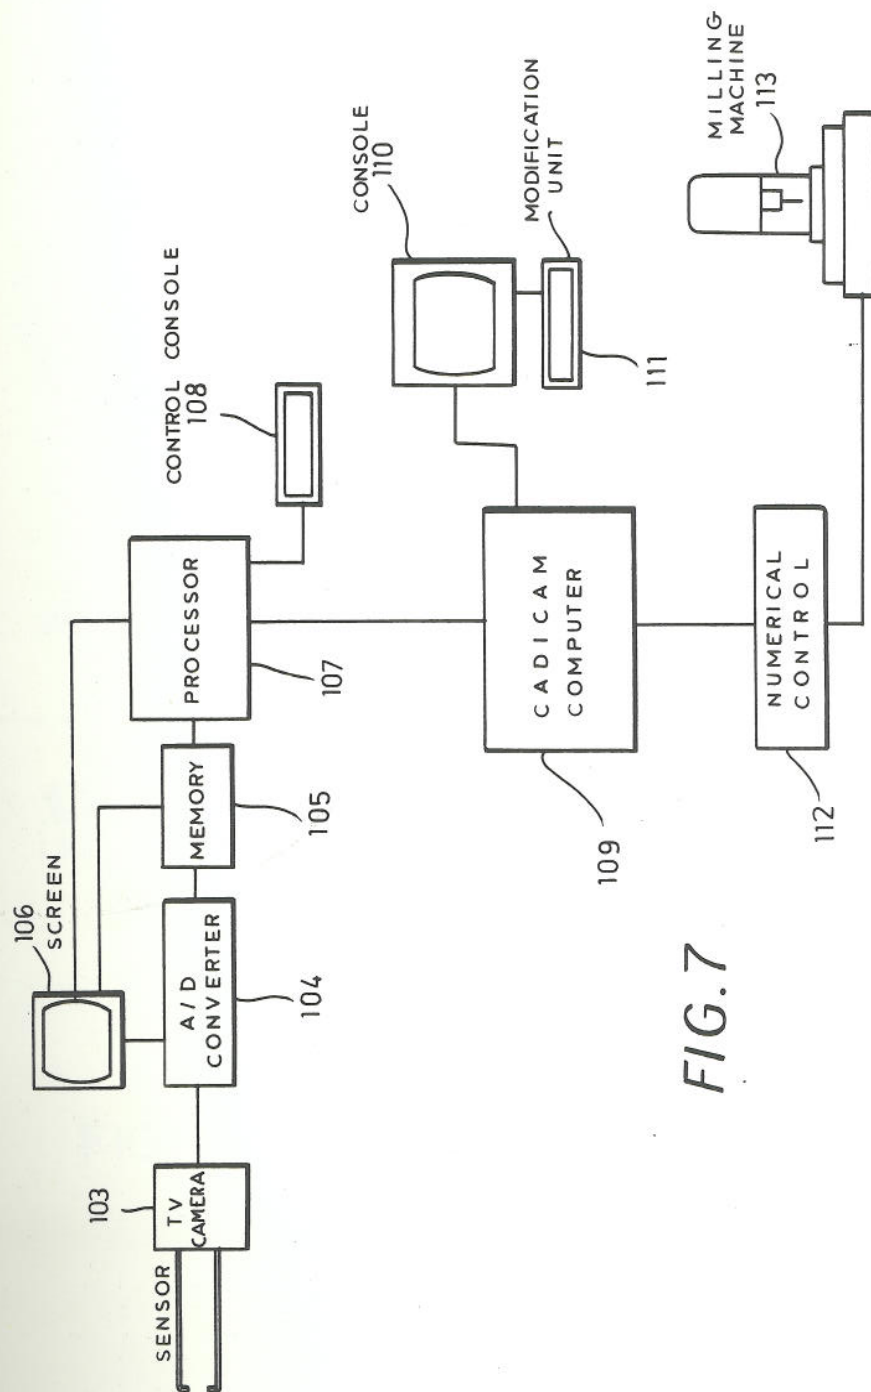


FIG. 7

FIG.9

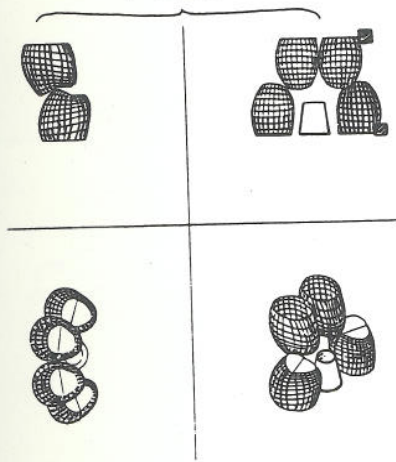


FIG.10

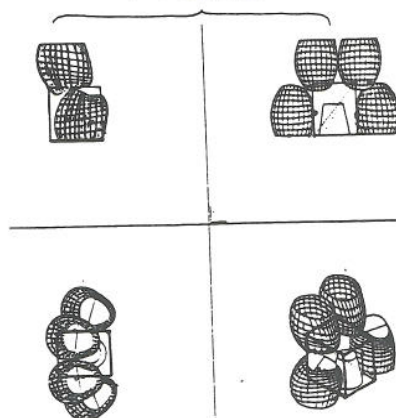


FIG.11

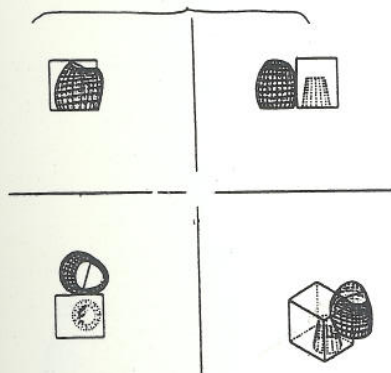


FIG.12

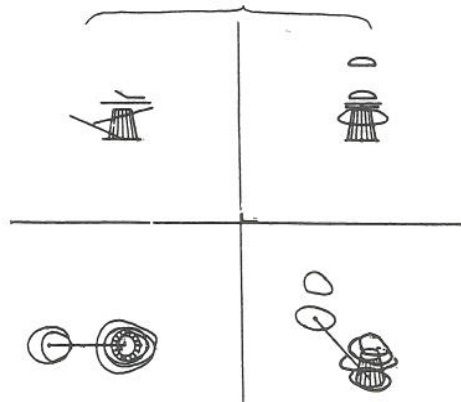
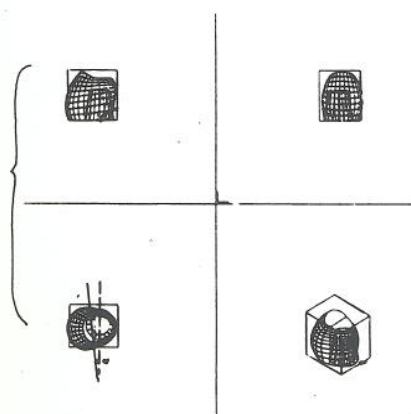


FIG.13



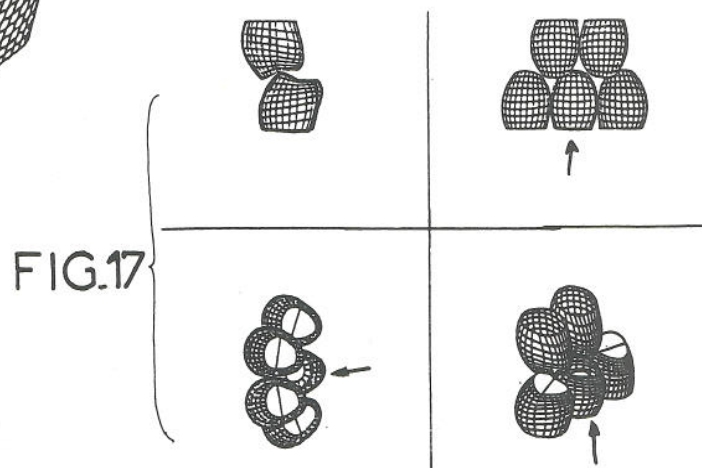
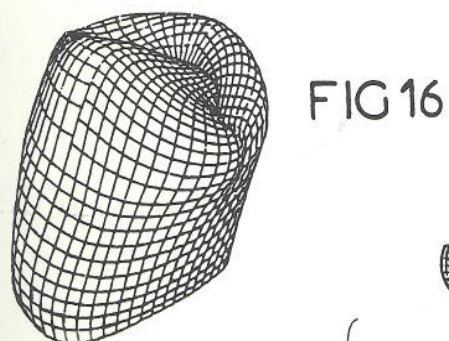
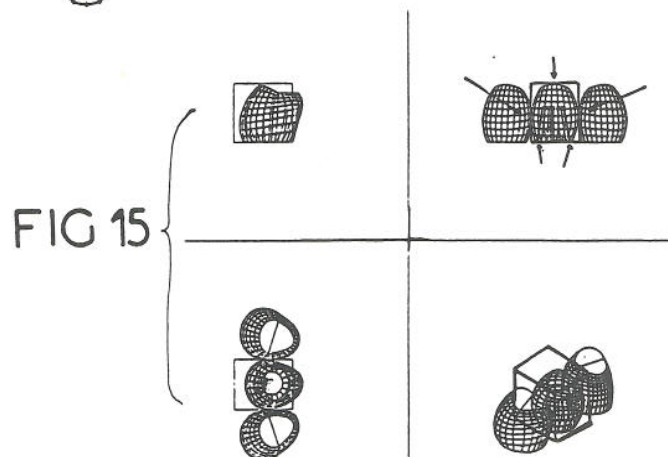
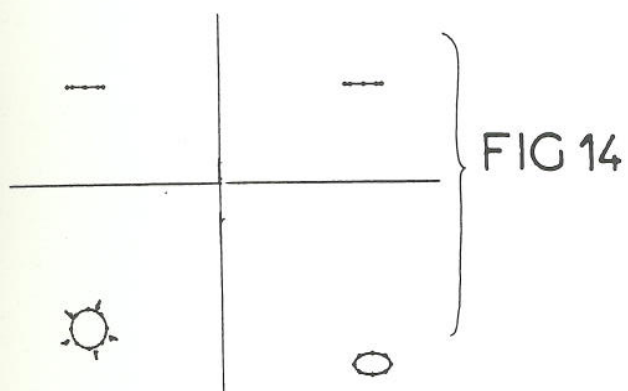


FIG.18

POINT NUMERO 1	X = 1.43 288	Y = 0.09 771	Z = -0.32 480
POINT NUMERO 2	X = 1.47 239	Y = -0.03 849	Z = -0.32 482
POINT NUMERO 3	X = 1.54 654	Y = -0.14 095	Z = -0.32 481
POINT NUMERO 4	X = 1.64 498	Y = -0.20 727	Z = -0.32 480
POINT NUMERO 5	X = 1.75 752	Y = -0.23 679	Z = -0.32 480
POINT NUMERO 6	X = 1.87 423	Y = -0.23 033	Z = -0.32 480
POINT NUMERO 7	X = 1.98 552	Y = -0.19 006	Z = -0.32 480
POINT NUMERO 8	X = 2.08 213	Y = -0.11 948	Z = -0.32 480
POINT NUMERO 9	X = 2.15 522	Y = -0.02 340	Z = -0.32 480
POINT NUMERO 10	X = 2.19 637	Y = 0.09 211	Z = -0.32 480
POINT NUMERO 11	X = 2.19 768	Y = 0.21 962	Z = -0.32 481
POINT NUMERO 12	X = 2.15 205	Y = 0.35 027	Z = -0.32 481
POINT NUMERO 13	X = 2.04 011	Y = 0.50 696	Z = -0.32 482
POINT NUMERO 14	X = 1.92 823	Y = 0.61 991	Z = -0.32 480
POINT NUMERO 15	X = 1.82 272	Y = 0.68 935	Z = -0.32 480
POINT NUMERO 16	X = 1.72 603	Y = 0.72 258	Z = -0.32 482
POINT NUMERO 17	X = 1.63 922	Y = 0.72 591	Z = -0.32 481
POINT NUMERO 18	X = 1.56 338	Y = 0.70 243	Z = -0.32 480
POINT NUMERO 19	X = 1.50 010	Y = 0.65 231	Z = -0.32 480
POINT NUMERO 20	X = 1.45 169	Y = 0.57 233	Z = -0.32 480
POINT NUMERO 21	X = 1.42 147	Y = 0.45 562	Z = -0.32 482
POINT NUMERO 22	X = 1.41 385	Y = 0.29549	Z = -0.32 480

FIG.19


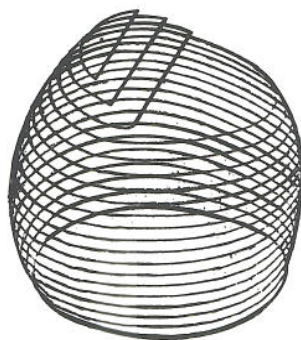


FIG.20



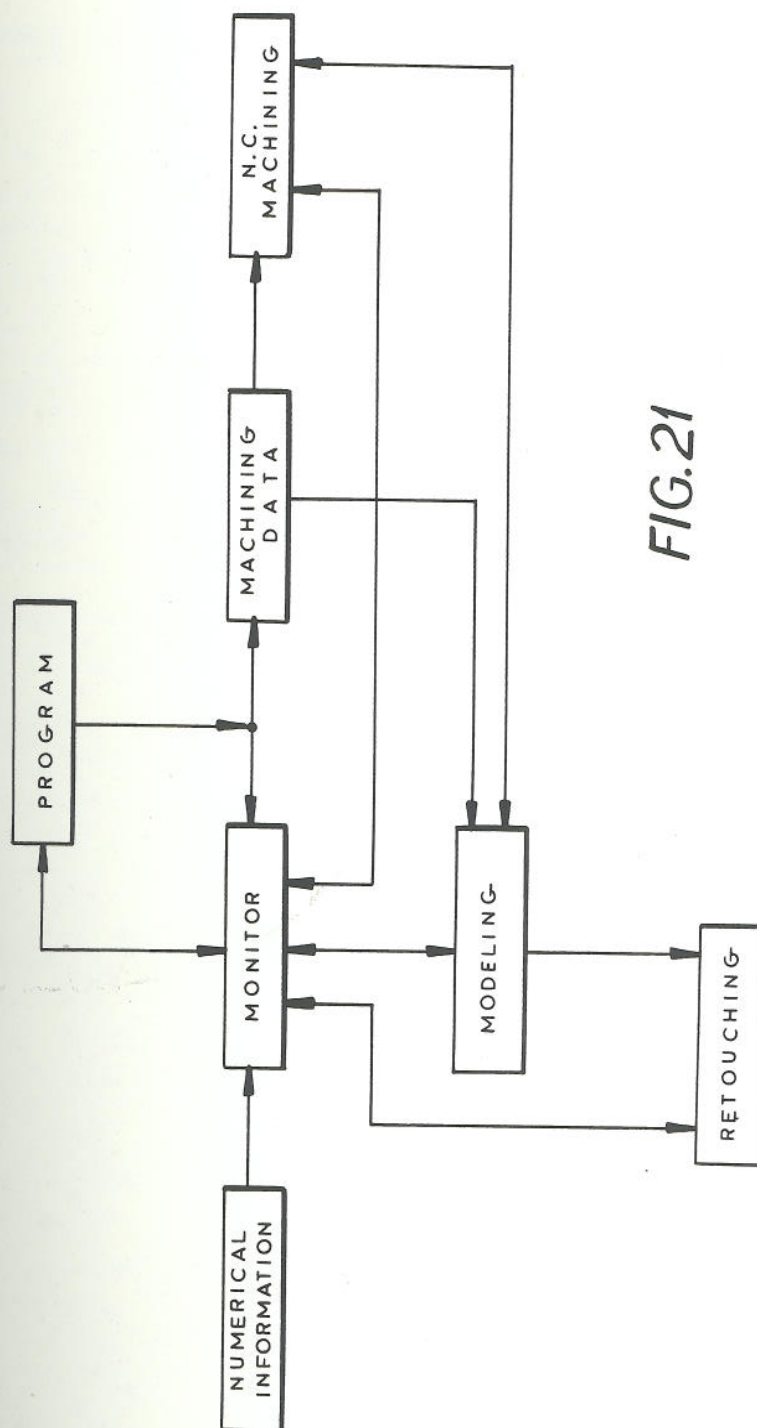


FIG. 21

METHOD OF AND APPARATUS FOR MAKING A PROsthESIS, ESPECIALLY A DENTAL PROsthESIS

CROSS REFERENCE TO RELATED APPLICATION

This application is a continuation-in-part of Ser. No. 60,776 filed Feb. 21, 1984 as a continuation of No. 62,905 filed May 12, 1981, both now abandoned.

FIELD OF THE INVENTION

Our present invention relates to a method of and to an apparatus for the making of a prosthesis and especially dental prosthesis. More particularly, this invention relates to a system for making a dental prosthesis in which, after preparation of the site in the mouth, the dental practitioner need only develop an electronic impression of this site as the sole intervention step before inserting the completed prosthesis.

BACKGROUND OF THE INVENTION

The aforementioned application points out that earlier methods of making dental prostheses, e.g. crowns, plates and replacement teeth, involved a multiplicity of steps, many of which required intervention in the mouth of the patient.

Not only was the patient required to attend the dental practitioner a comparatively large number of times but frequently the intervention was painful, especially during the fitting stages.

In the formation of a dental crown, for example, the operations include the grinding of the tooth to be replaced in order to obtain a truncated stump, the taking of an impression of the stump using an elastomeric path in order to obtain a mold whose hollow part has a shape which is complementary to that of the stump, the casting of plaster into said mold in order to obtain a reproduction of the stump, the preparation of the crown in wax taking into consideration adjacent and antagonistic teeth (a process which was generally highly subjective and the effect of which required high skill and long years of experience by the practitioner), the positioning of the crown in a coating cylinder, the melting out of the wax, the injection of molten metal to replace the wax, stripping and polishing of the metal crown, and, setting of the crown on the stump.

In spite of the fact that these numerous operations were carried out by highly skilled and fastidious dental surgeons, frequently modification of the prosthesis was required after the formation.

Indeed, because of the large number of steps which were involved and the fact that even with mechanical impressions, accurate fits could not be ensured, and because the relationship of each prosthesis to the adjacent and antagonistic teeth was something which had to be gauged subjectively by the practitioner, the production of a dental prosthesis hitherto seldom could be accomplished without the many visits mentioned previously. Indeed, in spite of numerous fitting operations, there was always the danger that the finished prosthesis would cause discomfort to the patient.

Another disadvantage of the earlier systems should also be apparent. For example, the metals used had to be fluid or malleable at easily obtainable temperatures. The numerous steps required the intervention of a laboratory and skilled practitioners at different stages in addition to the dental surgeon. The equipment required

overall, including an oven, sand-blasting machine, inserting equipment, contributed substantially to the cost of producing the prosthesis.

Because the temperature to which the materials were subjected, ranged from room temperature at which some work was done to the casting temperature, to the body temperature of the patient, uncontrolled thermal expansion posed a problem.

In the production of other prostheses, it was necessary to utilize a so-called "bloody impression" when, for example, an impression was required from injured bone. This involved pain and required especially sterile surgical procedures and handling of the impression media. Obviously, repeated fits here were an even more severe drawback.

OBJECTS OF THE INVENTION

It is, therefore, a principal object of the present invention to provide an improved method of and apparatus for the production of a prosthesis, and especially a dental prosthesis, whereby the numerous interventions with respect to the body of the patient can be eliminated and indeed many, if not all, of the drawbacks of the earlier systems described can be obviated.

Another object of this invention is to provide a method and apparatus for the fabrication of a dental prosthesis which allows the fabrication of the entire prosthesis or at least a substantial portion thereof by a machining operation outside the mouth of the patient so that the disadvantages of casting techniques are obviated.

Still another object of this invention is to provide a method and apparatus which extends the principles set forth in the above mentioned copending application.

SUMMARY OF THE INVENTION

These objects and others which will become apparent hereinafter are attained, in accordance with the invention, in a method whereby an optical impression is taken of the prosthesis site in the mouth and provides an interferogram image of the region at which the prosthesis is to be positioned and its relationship with adjoining teeth and occlusive teeth so that this image can be quantified in terms enabling selection from a stored collection of tooth shapes and sizes in a best-fit approach.

According to the invention, utilizing the data obtained from the best-fit approach, i.e. from the stored data regarding the standard shape and the modifications required to conform the best-fit shape to the tangent place and occlusive conditions from the particular site, a blank is machined by a numerically controlled three-dimensional machine tool so that both the fit to the location and the relationship of the machined prosthesis to the adjoining structures are optimum and determined exclusively by the optical impression.

We have found that, utilizing a computer programmed for computer assisted design of three-dimensional objects to which the optical impression input is fed, and a machine tool of a numerically controlled type which is numerically controlled by this computer, a highly compact apparatus can be provided which allows the dental practitioner to carry out the computer fabrication operation at his office after seeing the patient only once for preparation of the site and the optical impression so that on the next visit the completed prosthesis may be applied. Indeed, since the entire operation

takes only a short period of time, a completed prosthesis may be provided while the patient waits.

While we have used the term "interferogram" to refer to the image received, this expression is used in its broadest sense to refer to the obtention of a three-dimensional or holistic image. The preferred mode of obtaining this image is by interferometry which will be discussed below, although laser holographic techniques may be used as well or in addition.

Consequently, the method of the invention takes an optical impression of that part of the body which is designed to receive the prosthesis, effects a numerical, analog, and, electric clock conversion of the impression into data which is processed taking into account the characteristics of the prosthesis to be obtained and in determining the shape of the latter and sculpturing the prosthesis three-dimensionally with a numerically controlled machine tool.

The process of the invention provides for completely automatic production of a prosthesis with the possibility of preserving with great accuracy the optical impression in all of its holistic aspects. Although the process requires relatively sophisticated and costly apparatus, since it requires a computer and a numerically controlled machine tool, it has the advantage of high precision in the production of the prosthesis and high speed production thereof because it eliminates all of the intermediate phases of earlier techniques.

By eliminating these intermediate phases and the equipment involved in them and because of the gain in time, the cost of the apparatus of the invention is readily amortized, especially since the computer, which is required for the process, can also be used for other purposes.

As noted, an interferogrammatic impression is taken and advantageously two wave sources can be used, namely, an object beam diffracted by the object (the prosthesis site) and a refracted reference beam to obtain the impression in the form of wave interference patterns which can be evaluated and broken down into increments forming the numerical or digital data processed by the computer.

Since the wave interference pattern carries in itself the notion of distance, a holistic image makes it possible to obtain an impression that will not be deformed and will remain intact when carried over via the computer to the machine tool.

In accordance with a first possibility, the interference pattern is generated on a holographic plate while in another possibility the patterns or information are scanned directly utilizing a numerical, analog or electric analog converter.

The impression can advantageously be obtained by projection onto the organ or site to be provided with the prosthesis of a perfectly monochromatic laser wave which does not traumatize the tissue having a power, for example of 100 millijoule. Preferably an interference grating pattern can be projected and this need not use a coherent light source.

The impression can be taken on visible or exposed organs such as two stumps when the prosthesis is a dental crown or even through some media such as the skin or body tissues in order to obtain the impression of subjected organs for osteosynthesis prosthesis without the need for bloody impression techniques.

In a preferred mode of operation, the computer is preprogrammed to contain in memory detailed information regarding the possible prosthesis to be manufac-

tured. This can include information regarding the shape of the prosthesis, e.g. standard tooth shapes, information relating to relationships of the prosthesis to adjacent and antagonistic structures (e.g. information regarding an adjoining tooth and antagonistic tooth) and even information regarding the details of attachment of the prosthesis to the implantation site (e.g. adhesive clearances).

The three-dimensional impression of the site is then automatically quantified in the manner described and stored in the computer which can call up the stored data regarding the location, standard tooth shapes and sizes and the like enabling the best-fit of the tooth or teeth to that locus.

The teeth can be displayed on a screen of a video monitor or CRT associated with the computer to allow selection by the dental practitioner. After the selection is made from the stored data regarding the selection, the tooth sizes may be modified in view of the occlusive place and the adjacent structures automatically in accordance with preprogrammed information in the computer and the result is completed with the data of the stump and the site to enable an information set to be provided to the machine tool for the precise three-dimensional sculpturing of the finished prosthesis from a material as assisted by the operator.

The invention will be further described with reference to the manufacture of a dental crown. This is to be considered a preferred, but by no means exclusive embodiment.

In accordance with the invention, data roughly describing a plurality of standard teeth is stored in a computer. Data of at least 32 adult teeth, 20 baby teeth and possibly some other teeth of special shape must be stored.

Next, an optical image of the implantation site of the prosthesis is obtained. Specifically, the image is obtained by first projecting a luminous grating onto the implantation site.

The grating deformed in accordance with the shape of the site. Interference patterns are then created between the so-deformed grating and a reference grating.

The interference between the two gratings results in the appearance of interference fringes. Interference patterns consisting of the fringes are subjected to analog-digital conversion and the resulting values are stored in the computer. The computer then controls a machine tool which manufactures the prosthesis without any further need to inconvenience the patient and, further, without any need for manual intervention by the doctor or dentist concerned.

BRIEF DESCRIPTION OF THE DRAWING

The above and, other objects, features and advantages will become more readily apparent from the following description reference being made to the accompanying drawing in which:

FIGS. 1-4 are interference patterns of four surfaces of one tooth;

FIG. 5 is a block diagram of the system of the present invention;

FIG. 6 is a schematic diagram illustrating the apparatus for creating interference patterns of a tooth;

FIG. 7 is a block diagram of the apparatus linking the interference pattern readout to the machine tool apparatus;

FIG. 8 illustrates views to create a z (computer assisted data) of the prosthesis;

FIG. 9 illustrates faces of the prosthesis;

FIG. 10 illustrates the space into which the prosthesis is to be placed;

FIG. 11 illustrates the space of the prosthesis;

FIG. 12 illustrates the standard tooth implantation zone;

FIG. 13 illustrates the faces of the standard prosthesis;

FIG. 14 illustrates the plane of the modified prosthesis;

FIG. 15 illustrates the plane of the modified prosthesis;

FIG. 16 illustrates the plane of the modified prosthesis;

FIG. 17 shows the plane of the modified prosthesis;

FIGS. 18, 19 and 20 show the plane of the modified prosthesis;

FIG. 21 is a functional block diagram of the system.

SPECIFIC DESCRIPTION

The present invention relates to the manufacture of a prosthesis. It is noted that the invention involves the use of computer types of prosthetic design and manufacturing equipment in the utilization of CAM equipment in the manufacture of a prosthesis.

Setting up the computer for the present invention involves the use of a computer which must further be noted, though not operationally, requires a person skilled in the utilization of CAM equipment in the manufacture of a prosthesis.

The data defining the prosthesis is entered into the computer in numerical form. The x , y and z coordinates of a point on the prosthesis are defined, and lines, circles, etc. are mathematically defined.

(CAD) suitable for "EUCLID AND 3D CAD, of the Digital Equipment Corporation.

It should be noted that the rough or standard tooth and need not be represented by a standard tooth.

After the dentist has decided on the shape of the prosthesis in the mouth, the dentist proceeds to project a light onto the implantation site with either a grating deforms in the mouth so that interference patterns are created on the so-deformed grating, not deformed.

FIG. 8 illustrates the combination of a plurality of views to create a three-dimensional model by CAD (computer assisted design);

FIG. 9 illustrates four views of the implantation zone of the prosthesis;

FIG. 10 illustrates the actual planes limiting the volume into which the prosthesis must be inserted;

FIG. 11 illustrates the fitting of a standard tooth derived from computer memory into the volumetric space of the prosthesis;

FIG. 12 illustrates movement of the center of gravity of the standard tooth onto the center of gravity of the implantation zone;

FIG. 13 illustrates deformation of the external surfaces of the standard tooth to fit into the volume of the prosthesis;

FIG. 14 illustrates the cement film on which the prosthesis is to be held;

FIG. 15 illustrates the superposition of the bottom plane of the modified standard tooth with the corresponding plane of the implantation site;

FIG. 16 illustrates the actual model of the prosthesis which has been derived from the standard model stored in the computers;

FIG. 17 shows four views of the final prosthesis in place;

FIGS. 18, 19 and 20 illustrate the machining of successive planes under program control; and

FIG. 21 is a function diagram for the apparatus of FIG. 7.

SPECIFIC DESCRIPTION

The present invention will be discussed with regard to the manufacture of a crown for a tooth. It should be noted that the invention can be equally used for other types of prosthetic devices such as osteosynthetic. It must further be noted that understanding of the invention, though not operation of the resulting equipment, requires a person skilled in the art of Computer Aided Design and Manufacture (CAD/CAM). Specifically, skill in the utilization of commercially available CAD/CAM equipment is essential.

Setting up the computer so that the method of the present invention may be used, in the case of a dental prosthesis involves the insertion into memory of data roughly defining 32 adult teeth, 20 baby teeth and, as required, additional teeth having odd shapes.

The data defining the shape of each of the above-mentioned teeth is entered into the memory of the computer in numerical form. Each tooth is defined by x, y, z coordinates of a plurality of points, as well as by a number of reference values, such as the center of gravity, and lines, circles or surfaces which may be mathematically defined. A computer aided design system (CAD) suitable for this purpose is, for example, the "EUCLID AND VAX" (Geometric Construction), CAD, of the Digital Equipment Corp.

It should be noted that this entry into memory of rough or standard tooth shapes is a one time operation and need not be repeated for each patient.

After the dentist has prepared the site of implantation of the prosthesis in the conventional manner, he proceeds to project a luminous grating onto the implantation site with either coherent or non-coherent light. The grating deforms in dependence on the shape of the site, so that interference fringes are created between the so-deformed grating and a reference grating which is not deformed.

FIGS. 1-4 are examples of so-created patterns. The interference patterns illustrated in FIGS. 1-4 correspond to four optical recordings of four faces of a tooth.

Reading out of the images may take place after recording on a holographic plate or other suitable recording medium or, preferably, directly by a television camera or a plasma display.

This is illustrated generally by steps 20 and 30 in FIG. 5. FIG. 6 illustrates a light source, 101, projecting a grating onto the tooth site. The grating is correspondingly deformed and an interference pattern, 102, created by superimposition of an undeformed reference grating.

The pattern is scanned by a TV camera 103. Plane 104 represents an interference plane. The pickup can be in a video camera or a CCD (chargecoupled device) camera.

The equipment linking the camera sensor to the final machine tool, for example a milling machine, is illustrated in FIG. 7. A television camera 103 scans the interference pattern. An analog/digital converter 104 converts the scanned data and stores it in memory. The image is also projected onto a cathode ray screen 106. The image on the screen is subjected to processing for purposes of simplification, as will be explained in greater detail below. For this purpose, the operator controls a control console 108 which, in turn, controls an image processor 107. After the image has been processed, it is subjected to computer-aided design in a computer 109, also to be described in greater detail below. The output of computer 109 is displayed on a suitable screen 110, the image on which may be modified by operation of a modification unit 111. The final output of the computer is numerical control data which, through a numerical control unit 112 controls the final machine tool, here a micro-milling machine 113 (see also FIG. 21). Processing of the interference patterns proceeds as follows:

The interference patterns have certain contour lines which are a function of the volume of the tooth.

For any point, the xy coordinates are obtained by direct read-out. The third coordinate, z, can easily be calculated with the aid of a formula giving the distance h between two interference fringes;

$$h = 2aD^2/bF$$

As illustrated in FIG. 5:

F is the focal distances;

b is the distance between the transmitting and receiving objectives;

a is the spacing between grating lines;

and D is the distance between the apparatus and the interference plane.

The third coordinate z is given by the formula

$$a = (2aD^2/bF)n$$

where n represents the number of fringes.

Before the proceeding to determine the different coordinates of each point, the image is reduced to a skeletal version so that the number of reference values of z is the least possible. This is accomplished by reducing the number of points in each curve and reducing the number of curves, keeping in mind the minimum degree of accuracy which must be preserved.

Preferably, the coordinates of each point are obtained using FORTRAN, for example FORTRAN 22, by which, for each value of z, the corresponding values of x and y are found.

The analog/digital conversion of the data takes place very simply by counting of fringes or by sinusoidal interpolation between fringes. It is considered that a fringe is black and that the space between fringes is white. After the simplification, each fringe corresponds to a black line of several microns. The value 0 is assigned to each black point, while the value 1 is applied to each white point. The formula mentioned above then can be used to determine the value of z correctly. The values of x and y are given by the position of the point being analyzed on the image plane.

All these operations are carried out by the computer which, for this purpose, is equipped especially with commercially available programs such as VAX730 of the Digital Equipment Corporation or with booting or operating cards such as Thompson CSF (31138 ANB-TIBLOWING) and associated Program (THX 5002: Frequency Generator and Command Logic, and THX 5003: Video channel and analog digital conversion).

To the extent that the implantation site and the adjacent areas of the prosthesis necessitate views from different angles, the computer will reconstitute the overall shape of the site by combining such views as is illustrated in FIG. 8. This figure was obtained by the Euclid and Vax, FUSION design package.

Next, the determination of the volume (envelope) of the prosthesis must be carried out.

This is a two-step operation.

(a) imaging of the implantation zone of the prosthesis; (FIG. 9 shows this zone from four angles);

(b) adaptation of the standard form or rough outline of the tooth stored in the computer memory to the visualized shape of the prosthesis.

First, the operator causes an area to appear on a cathode ray screen into which the standard form of a theoretical tooth in the memory is inserted. This volume is parallelepiped and is obtained by geometric determination of 6 planes, taking into consideration the contact zones with the neighboring teeth (planes 1 and 2), the front and rear faces of the neighboring teeth (planes 3 and 4) the contacting surface of the opposite teeth (plane 5) and finally the lower limit of the implantation zone of the prosthesis (plane 6). This defines the real limits of the volume into which the prosthesis must be inserted (FIG. 10).

To avoid having to enter excessive data into the computer, the prosthesis is generated by adaptation of a standard tooth shape in the computer memory to fit into this volume.

As mentioned above, the operator first causes the theoretical tooth stored in the memory which is closest to the tooth to be fitted to appear on the screen (FIG. 11). By using a CAD/CAM package (Euclid: Geometric Transformation), and by controlling the cathode ray tube, the operator matches the form of the theoretical tooth to the previously determined volume or envelope. This adaptation is first made by moving the center of gravity of the standard tooth onto the center of gravity of the implantation site of the prosthesis (FIG. 12), then by deformation of the surfaces of the outline of the standard tooth, so that they are tangent to the planes limiting the volume of the previously determined envelope (FIG. 13).

The exterior surface of the prosthesis has thus been defined. The interior (lower) surface corresponds to that of the implantation site. The logic package (Euclid) then determines the actual volume of the prosthesis, taking into consideration the exterior surface previously

defined, the shape of the implantation site, and finally, other factors such as the thickness of the cement film which will hold the prosthesis (FIG. 14). The combination of interior and exterior surfaces is effected by superposition of the implantation site on the lower limit of the standard tooth, as modified (FIG. 15).

The computer aided design system, such as Euclid and VAX, allows the transformation of the theoretical model into the actual model (FIG. 16). The results can be visualized according to predetermined views (FIG. 17). At this stage, visualization of the actual model of the prosthesis and its adjoining areas make it possible to verify the exact shape of the model and, if necessary, make modifications at particular points.

After the real model has thusly been determined, the CAD/CAM system controls the manufacture of the prosthesis or, depending upon the material utilized, of a casting into which the material for the prosthesis will be poured. FIG. 18 illustrates the program for manufacturing control of successive planes, as generated by Euclid. (FIGS. 19 and 20).

The process of the present invention thus has several principal stages which may be summarized as follows:

(a) one time creation of an optical pattern independently of the object itself and connected only to an interference phenomenon, either optical-optical or optical-electronic;

(b) immediate carrying out of an analog-digital conversion;

(c) determining the external and internal shape of the prosthesis solely by mathematical means within the computer, on the basis of CAD/CAM techniques, the computer having stored data defining standard shapes, such as the shape of the adult and baby teeth, which may be modified in accordance with the interference patterns derived from the particular patient.

It must be noted that nowhere in the process of the present invention is wax or resin used to make an imprint nor is there any manual adjustment of the prosthesis.

The process has been carried out successfully by the inventors to manufacture a prototype which functions perfectly and which allowed a dental prosthesis to be manufactured within 20 minutes.

It must of course be understood that, in particular, the process of the present invention makes use of a truly interferometric method. In a preferred embodiment, the interference patterns are not obtained by interference of a reference beam and a diffraction beam, but by interference between a grating which is not deformed and a luminous grating which is deformed by the zone being analyzed. It should be noted that it is not measurements of an object, but solely interference phenomena derived from the object which are utilized in the automatic manufacture of the prosthesis.

This interferometric method allows analog-digital conversion with the restricted financial means available in a, for example, dental office. The shape of the prosthesis is then derived strictly mathematically by a CAD/CAM system.

Further, the interferometric method allows the optical interference patterns to be obtained in a very short time, namely several microseconds (scanning at 5 MHz), data processing taking place in several seconds, as opposed to other methods which require either a long readout time for a short data processing time or a short readout time but a long processing time (30 minutes to an hour) with very powerful computers which are not

financially within office.

We claim:

1. A method of comprises, carrying, the steps of:

creating an inter-
corresponding
in the buccal
scanning said in-
site data;
processing said c
data;
machining said p
cal cavity dir
tool data, said
plurality of st
and
wherein said s

comprises g
volume of
data, displa
lecting from
terns the pa
said organ,
tern, and fit
lope under
desired sha
puter comp
said selectec
create said

2. A method as s
of processing said
modification of sa
upon the material

3. Apparatus for
determined organ
means for creati
site data cor
view of said c
means for scanni
verting said sc
computer means
verting means
said digital si
under operato
sis shape and
shape into ma

financially within the reach of, for example, a dental office.

We claim:

1. A method of producing a dental prosthesis which comprises, carrying out under the control of a computer the steps of:

creating an interference pattern containing site data corresponding to a three-dimensional view of a site in the buccal cavity;

scanning said interference pattern to produce digital site data;

processing said digital site data to create machine tool data;

machining said prosthesis to fit said site and said buccal cavity directly under control of said machine tool data, said computer having a memory having a plurality of standard tooth patterns stored therein; and

wherein said step of processing said digital site data comprises generating an envelope enclosing the volume of said prosthesis from said digital site data, displaying the so-produced envelope, selecting from said plurality of standard tooth patterns the pattern corresponding most closely to said organ, displaying the so-selected tooth pattern, and fitting said tooth pattern into said envelope under operator control, thereby creating a desired shape display, and wherein said computer computes said machine tool data based on said selected standard tooth shape as modified to create said desired shape display.

2. A method as set forth in claim 1, wherein said step of processing said digital site data further comprises modification of said machine tool data in dependence upon the material of said prosthesis.

3. Apparatus for creating a prosthesis of an organ at a determined organ site, comprising:

means for creating an interference pattern containing site data corresponding to a three-dimensional view of said organ site;

means for scanning said interference pattern and converting said so-scanned pattern to digital site data;

computer means connected to said scanning and converting means for creating an optical image from said digital site data, and modifying said image under operator control to create a desired prosthesis shape and converting said desired prosthesis shape into machine tool data; and

machining means connected to said computer means for manufacturing said prosthesis under control of said machine tool data.

4. Apparatus as set forth in claim 3, wherein said prosthesis is a ground for a tooth;

wherein said computer further comprises a memory having a plurality of standard tooth patterns stored therein;

wherein said optical image is an envelope enclosing the volume of said prosthesis; and

wherein said modifying means comprises a selecting means for selecting one of said plurality of standard tooth patterns and adjusting said tooth pattern under operator control into said envelope, the so-modified standard tooth pattern constituting said desired prosthesis shape.

5. A method of making a dental prosthesis which comprises the steps of:

storing in a computer memory, data representing standard tooth shapes and sizes, relationships between teeth and adjacent and occlusive teeth and characteristics for securing a prosthesis to a prepared site, and machining instructions for shaping a blank to the configuration of a dental prosthesis for direct implantation;

preparing a site in the mouth of a patient to receive a dental prosthesis;

projecting optically a grating upon said site in the mouth of said patient and generating an interference pattern representing a holistic impression of said site and its relationship to adjacent structures; converting said interference pattern into data along x, y, z coordinates in a cartesian coordinate system representing machining of a blank to fit said site;

matching data obtained by said impression with said computer to standard prosthesis shapes and sizes and selecting a best-fit shape and size and modifying same in said computer to match said site;

numerically controlling said machine tool with said x,y,z coordinate data and x,y,z coordinate data from the match made by the computer and representing the shape and size of said prosthesis to totally and three-dimensionally fabricate said prosthesis in said machine tool; and

implanting the totally fabricated prosthesis at said site.

6. The method defined in claim 5 wherein said prosthesis is a dental crown.

7. The method defined in claim 6 wherein said pattern is skeletonized to reduce the number of points which are matched by the data stored in said computer.

* * * * *